



BOD

Frequency	Date Sample Obtained	Date Result Obtained	Unit of Measurement	EPA Limit	Sample Results
Monthly	05-Jun-24	13-Jun-24	milligrams per litre (mg/L)	MONITORING	2
Monthly	03-Jul-24	11-Jul-24	milligrams per litre (mg/L)		<2
Monthly	07-Aug-24	15-Aug-24	milligrams per litre (mg/L)		<2
Monthly	04-Sep-24	11-Sep-24	milligrams per litre (mg/L)		<2
Monthly	02-Oct-24	10-Oct-24	milligrams per litre (mg/L)		<2
Monthly	06-Nov-24	14-Nov-24	milligrams per litre (mg/L)	CONDITION	<2
Monthly	04-Dec-24	11-Dec-24	milligrams per litre (mg/L)		<2
Monthly	15-Jan-25	23-Jan-25	milligrams per litre (mg/L)		<2
Monthly	05-Feb-25	12-Feb-25	milligrams per litre (mg/L)		<2
Monthly	05-Mar-25	14-Mar-25	milligrams per litre (mg/L)		2
Monthly	09-Apr-25	16-Apr-25	milligrams per litre (mg/L)		<2
Monthly			milligrams per litre (mg/L)		

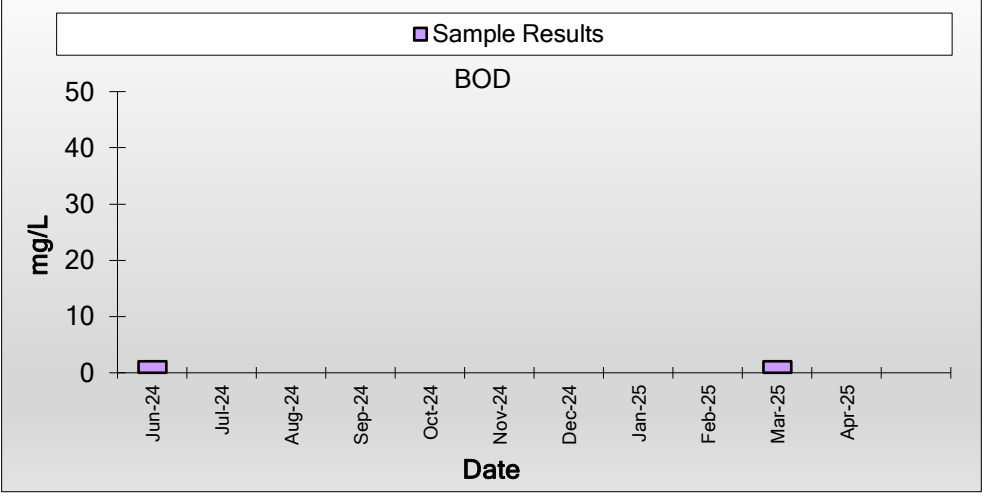


FAECAL COLIFORMS

Frequency	Date Sample Obtained	Date Result Obtained	Unit of Measurement	EPA Limit	Sample Results
Monthly	05-Jun-24	13-Jun-24	colony forming units per 100 millilitres (cfu/100mL)	MONITORING	<1
Monthly	03-Jul-24	11-Jul-24	colony forming units per 100 millilitres (cfu/100mL)		<1
Monthly	07-Aug-24	15-Aug-24	colony forming units per 100 millilitres (cfu/100mL)		<1
Monthly	04-Sep-24	11-Sep-24	colony forming units per 100 millilitres (cfu/100mL)		<1
Monthly	02-Oct-24	10-Oct-24	colony forming units per 100 millilitres (cfu/100mL)		<1
Monthly	06-Nov-24	14-Nov-24	colony forming units per 100 millilitres (cfu/100mL)	CONDITION	<1
Monthly	04-Dec-24	11-Dec-24	colony forming units per 100 millilitres (cfu/100mL)		<1
Monthly	15-Jan-25	23-Jan-25	colony forming units per 100 millilitres (cfu/100mL)		<1
Monthly	05-Feb-25	12-Feb-25	colony forming units per 100 millilitres (cfu/100mL)		<1
Monthly	05-Mar-25	14-Mar-25	colony forming units per 100 millilitres (cfu/100mL)		<1
Monthly	09-Apr-25	16-Apr-25	colony forming units per 100 millilitres (cfu/100mL)		<1
Monthly			colony forming units per 100 millilitres (cfu/100mL)		

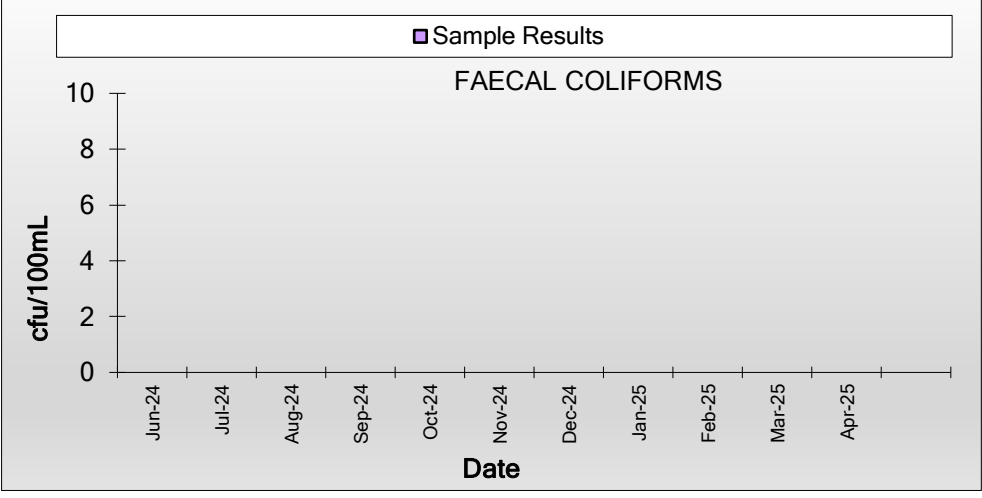


AMMONIA NITROGEN

Frequency	Date Sample Obtained	Date Result Obtained	Unit of Measurement	EPA Limit	Sample Results
Monthly	05-Jun-24	13-Jun-24	milligrams per litre (mg/L)	MONITORING	0.04
Monthly	03-Jul-24	11-Jul-24	milligrams per litre (mg/L)		0.08
Monthly	07-Aug-24	15-Aug-24	milligrams per litre (mg/L)		0.04
Monthly	04-Sep-24	11-Sep-24	milligrams per litre (mg/L)		0.07
Monthly	02-Oct-24	10-Oct-24	milligrams per litre (mg/L)		0.08
Monthly	06-Nov-24	14-Nov-24	milligrams per litre (mg/L)	CONDITION	0.14
Monthly	04-Dec-24	11-Dec-24	milligrams per litre (mg/L)		0.04
Monthly	15-Jan-25	23-Jan-25	milligrams per litre (mg/L)		0.02
Monthly	05-Feb-25	12-Feb-25	milligrams per litre (mg/L)		0.06
Monthly	05-Mar-25	14-Mar-25	milligrams per litre (mg/L)		0.04
Monthly	09-Apr-25	16-Apr-25	milligrams per litre (mg/L)		0.19
Monthly			milligrams per litre (mg/L)		

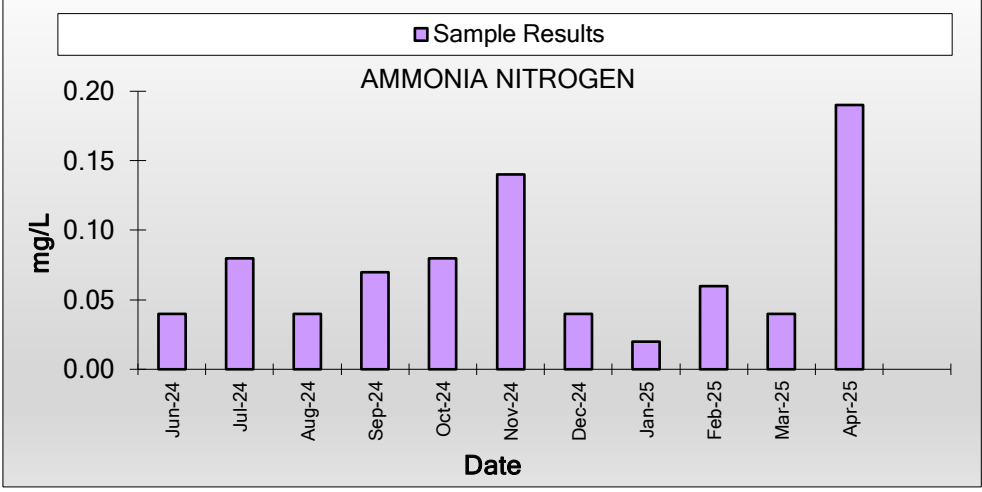


TOTAL NITROGEN

Frequency	Date Sample Obtained	Date Result Obtained	Unit of Measurement	EPA Limit	Sample Results
Monthly	05-Jun-24	13-Jun-24	milligrams per litre (mg/L)	MONITORING	1.3
Monthly	03-Jul-24	11-Jul-24	milligrams per litre (mg/L)		1.8
Monthly	07-Aug-24	15-Aug-24	milligrams per litre (mg/L)		0.9
Monthly	04-Sep-24	11-Sep-24	milligrams per litre (mg/L)		0.7
Monthly	02-Oct-24	10-Oct-24	milligrams per litre (mg/L)		0.8
Monthly	06-Nov-24	14-Nov-24	milligrams per litre (mg/L)	CONDITION	2.2
Monthly	04-Dec-24	11-Dec-24	milligrams per litre (mg/L)		5.2
Monthly	15-Jan-25	23-Jan-25	milligrams per litre (mg/L)		0.8
Monthly	05-Feb-25	12-Feb-25	milligrams per litre (mg/L)		1.8
Monthly	05-Mar-25	14-Mar-25	milligrams per litre (mg/L)		1.3
Monthly	09-Apr-25	16-Apr-25	milligrams per litre (mg/L)		0.8
Monthly			milligrams per litre (mg/L)		

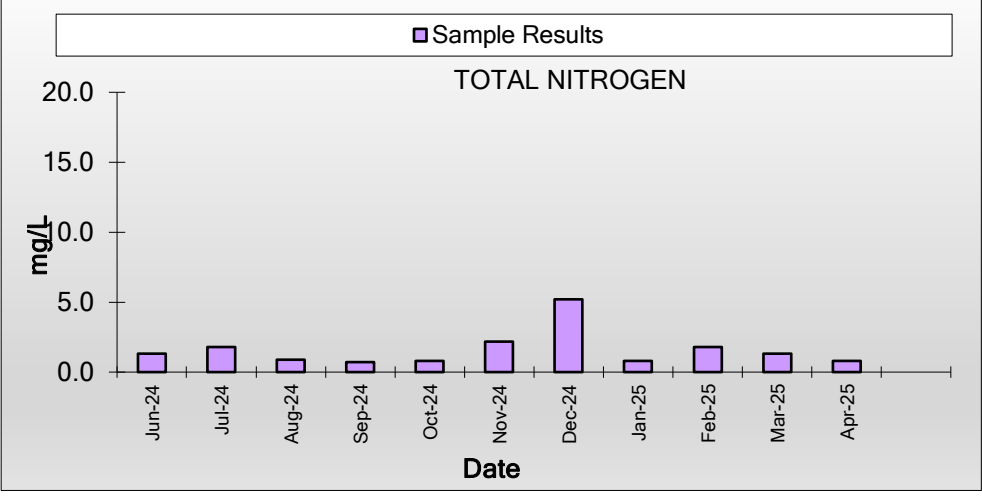


OIL AND GREASE

Frequency	Date Sample Obtained	Date Result Obtained	Unit of Measurement	EPA Limit	Sample Results
Monthly	05-Jun-24	13-Jun-24	milligrams per litre (mg/L)	MONITORING	<1
Monthly	03-Jul-24	11-Jul-24	milligrams per litre (mg/L)		<1
Monthly	07-Aug-24	15-Aug-24	milligrams per litre (mg/L)		<1
Monthly	04-Sep-24	11-Sep-24	milligrams per litre (mg/L)		<1
Monthly	02-Oct-24	10-Oct-24	milligrams per litre (mg/L)		<1
Monthly	06-Nov-24	14-Nov-24	milligrams per litre (mg/L)	CONDITION	<1
Monthly	04-Dec-24	11-Dec-24	milligrams per litre (mg/L)		<1
Monthly	15-Jan-25	23-Jan-25	milligrams per litre (mg/L)		<1
Monthly	05-Feb-25	12-Feb-25	milligrams per litre (mg/L)		<1
Monthly	05-Mar-25	14-Mar-25	milligrams per litre (mg/L)		<1
Monthly	09-Apr-25	16-Apr-25	milligrams per litre (mg/L)		<1
Monthly			milligrams per litre (mg/L)		

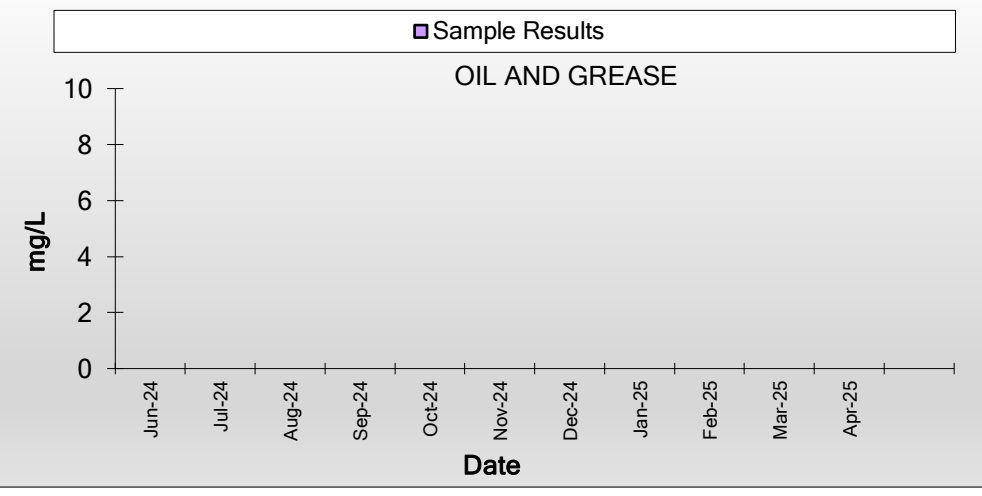


pH

Frequency	Date Sample Obtained	Date Result Obtained	Unit of Measurement	EPA Limit	Sample Results
Monthly	05-Jun-24	13-Jun-24	pH	MONITORING	7.6
Monthly	03-Jul-24	11-Jul-24	pH		7.7
Monthly	07-Aug-24	15-Aug-24	pH		7.6
Monthly	04-Sep-24	11-Sep-24	pH		7.6
Monthly	02-Oct-24	10-Oct-24	pH		7.5
Monthly	06-Nov-24	14-Nov-24	pH	CONDITION	6.9
Monthly	04-Dec-24	11-Dec-24	pH		7.5
Monthly	15-Jan-25	23-Jan-25	pH		7.6
Monthly	05-Feb-25	12-Feb-25	pH		7.4
Monthly	05-Mar-25	14-Mar-25	pH		7.3
Monthly	09-Apr-25	16-Apr-25	pH		7.4
Monthly			pH		

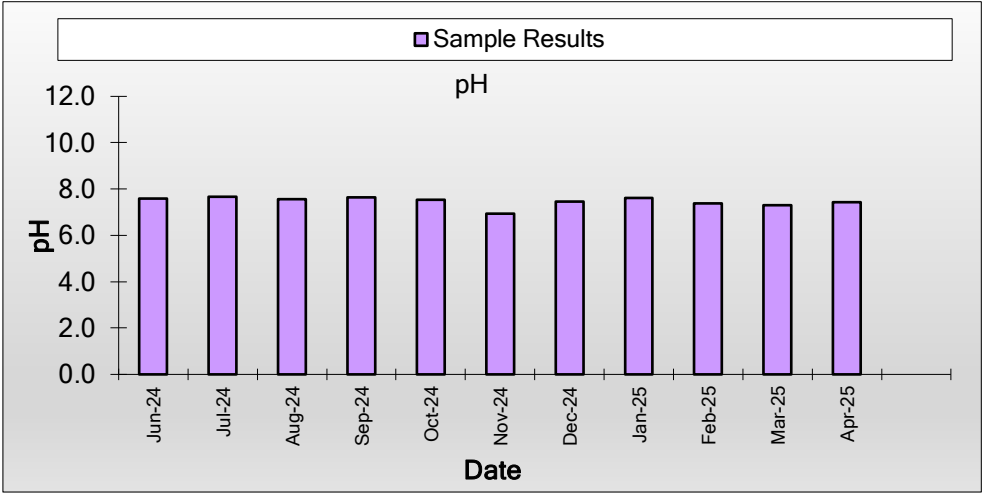


TOTAL PHOSPHORUS

Frequency	Date Sample Obtained	Date Result Obtained	Unit of Measurement	EPA Limit	Sample Results
Monthly	05-Jun-24	13-Jun-24	milligrams per litre (mg/L)	MONITORING	0.07
Monthly	03-Jul-24	11-Jul-24	milligrams per litre (mg/L)		0.15
Monthly	07-Aug-24	15-Aug-24	milligrams per litre (mg/L)		0.10
Monthly	04-Sep-24	11-Sep-24	milligrams per litre (mg/L)		0.16
Monthly	02-Oct-24	10-Oct-24	milligrams per litre (mg/L)		0.04
Monthly	06-Nov-24	14-Nov-24	milligrams per litre (mg/L)	CONDITION	0.15
Monthly	04-Dec-24	11-Dec-24	milligrams per litre (mg/L)		0.22
Monthly	15-Jan-25	23-Jan-25	milligrams per litre (mg/L)		0.15
Monthly	05-Feb-25	12-Feb-25	milligrams per litre (mg/L)		0.24
Monthly	05-Mar-25	14-Mar-25	milligrams per litre (mg/L)		0.21
Monthly	09-Apr-25	16-Apr-25	milligrams per litre (mg/L)		0.15
Monthly			milligrams per litre (mg/L)		

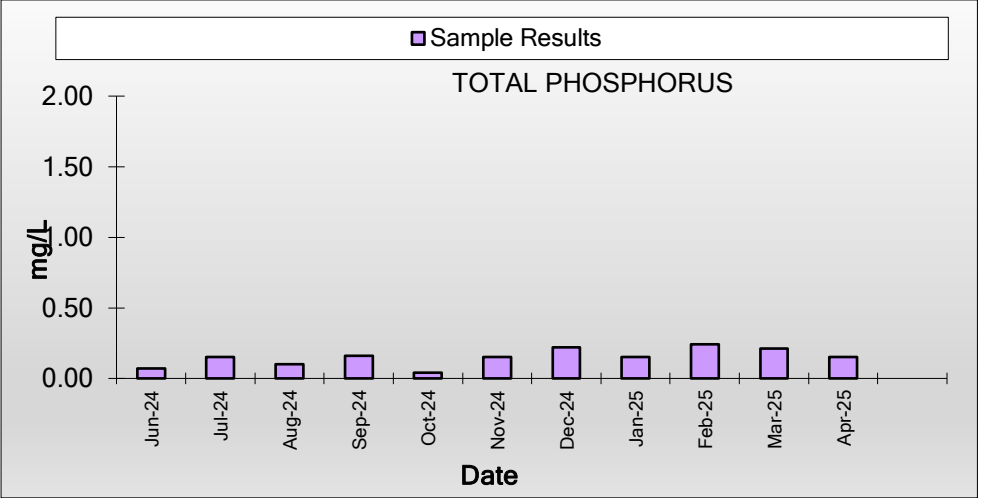

TOTAL SUSPENDED SOLIDS

Frequency	Date Sample Obtained	Date Result Obtained	Unit of Measurement	EPA Limit	Sample Results
Monthly	05-Jun-24	13-Jun-24	milligrams per litre (mg/L)	MONITORING	<1
Monthly	03-Jul-24	11-Jul-24	milligrams per litre (mg/L)		<1
Monthly	07-Aug-24	15-Aug-24	milligrams per litre (mg/L)		<1
Monthly	04-Sep-24	11-Sep-24	milligrams per litre (mg/L)		<1
Monthly	02-Oct-24	10-Oct-24	milligrams per litre (mg/L)		<1
Monthly	06-Nov-24	14-Nov-24	milligrams per litre (mg/L)	CONDITION	6
Monthly	04-Dec-24	11-Dec-24	milligrams per litre (mg/L)		2
Monthly	15-Jan-25	23-Jan-25	milligrams per litre (mg/L)		<1
Monthly	05-Feb-25	12-Feb-25	milligrams per litre (mg/L)		<1
Monthly	05-Mar-25	14-Mar-25	milligrams per litre (mg/L)		<1
Monthly	09-Apr-25	16-Apr-25	milligrams per litre (mg/L)		<1
Monthly			milligrams per litre (mg/L)		

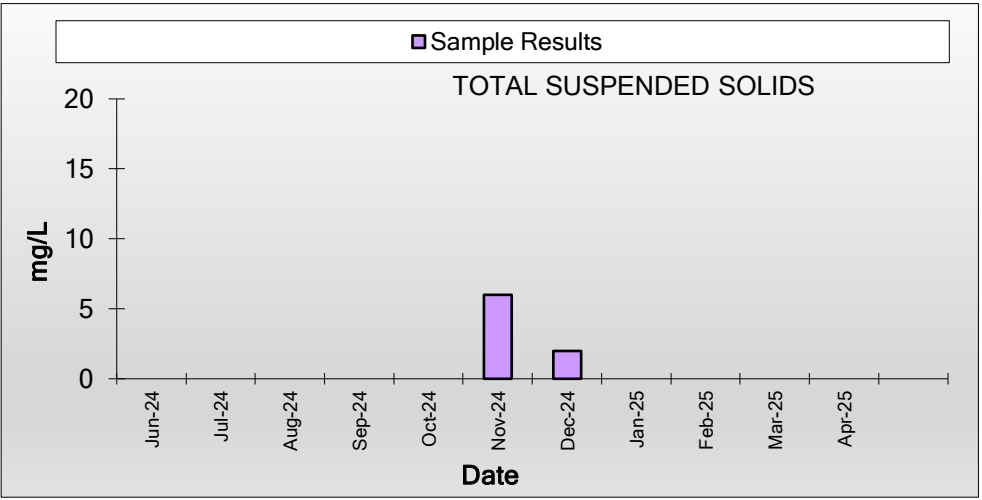

non-compliance notes: